



Upright Microscope ECLIPSE Ci/Ni

Nikon th
100
anniversary

ECLIPSE Ci/Ni

Upright Microscope



Feel the evolution

Nikon developed the clinical and laboratory microscope ECLIPSE Ci series to meet the demands of a microscope that provides comfortable posture during observation and simple set-up, such as magnification switching, light intensity reproduction and image capturing. With its small footprint, the Ci series delivers compact and space-saving observation conditions. Nikon also developed the ECLIPSE Ni series, which offers high optical quality and a wide range of imaging possibilities. The highly-evolved Ci/Ni series microscopes enable routine analysis with more comfort and greater flexibility than ever before.

ECLIPSE *Ci*

- **Eco Friendly**
High-intensity, long-life and power saving illumination
- **Ergonomic**
Flexible, adjustable design to suit the user's natural posture
- **Easy to Use**
One-touch operation for microscope* control and image capturing
- **Versatile**
Flexible observation with a wide range of specimens

*Ci-E

ECLIPSE *Ni*

- **High-quality**
Superior optical performance
- **Expandability**
Wide variety of optional motorized accessories
- **Automation***
Intelligent, automatic switching of observation methods

*Ni-E

● Meeting user needs in clinical microscopy

I want to easily capture images.

I want to conduct observation in comfort.

I want to observe images with bright and even illumination.

I want to simplify operation with motorized accessories.

I want to use a variety of observation techniques.

I want to reduce the number of lamp replacements.

ECLIPSE Ci

The Ci meets all your demands.

The ECLIPSE Ci series microscopes offer a bright field of view, high durability, comfortable posture for prolonged observation, simple motorized operation, and various illumination techniques that you need for clinical and laboratory microscopy.


Eco Friendly

● Eco-illumination (Ci-E/Ci-L)

The newly developed high luminescent LED is a low power consumption eco-friendly light source that produces evenly distributed illumination and reduces the cost and effort of lamp replacement thanks to its long-life.



Viewed with Eco-illumination



Viewed without Eco-illumination

*These images are captured without using the shading compensation to emphasize the vignetting.

● Ceramic-coated stage

The stage is coated with high durability scratch-resistant coating.



Ergonomic

● Ergonomic binocular tube

Eyepiece angle and extension are adjustable. A camera can be mounted via the DSC port.



Ergonomic binocular tube

● Eyelevel riser

Eye-point height can be adjusted to suit your natural posture and increases flexibility for multi-users of different heights.

● Lower stage positioning

Lower stage height using the nosepiece spacer for easy specimen exchange.



Nosepiece spacer

● Stage handle with height adjustment

Smooth stage movement is possible in a comfortable hand position.



Easy to use

- **Image capture button**

One simple click of the button during observation enables you to capture your specimen image with the Digital Sight camera.



- **Motorized magnification change (Ci-E)**

Magnification can be switched with one button control during observation, which automatically memorizes and reproduces user-defined light intensity.



- **DS-L4 Microscope Camera Control Unit**

The DS-L4's touch panel allows you to easily set and control your cameras as well as take simple measurements. It is also possible to switch the Ci-E's objective lenses.




Versatile

- **Flexible observation methods**

The high-intensity Eco-illumination and accessories enable you to perform phase contrast, darkfield and simple polarizing microscopy.

- **Image sharing**

The live image can be displayed on the DS-L4 monitor or via a projector. Simultaneous observation on networked PCs is also possible.

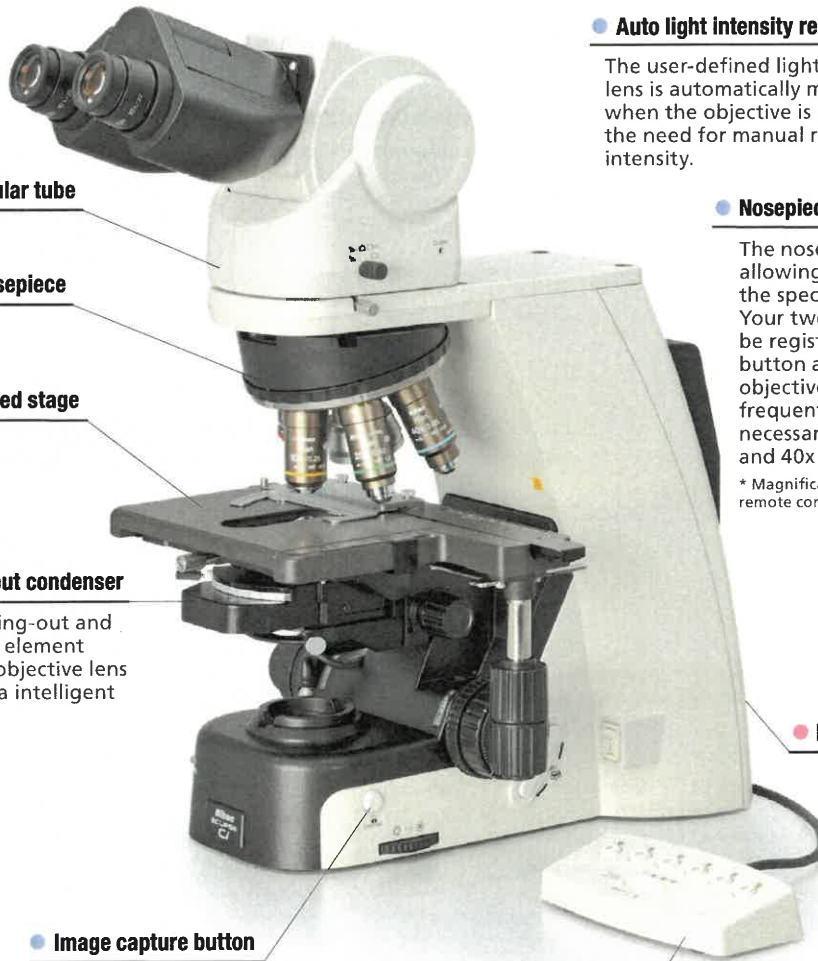

● **Ergonomic binocular tube**

● **Motorized nosepiece**

● **Ceramic-coated stage**

● **Motorized swing-out condenser**

Automatically swing-out and swing-in top-lens element according to the objective lens that is selected via intelligent linking.

● **Image capture button**

● **Remote control pad**

By programming specific buttons to correspond to specific objective lenses, magnification can be easily changed with a one-touch button.

● **Auto light intensity reproduction**

The user-defined light intensity for each objective lens is automatically memorized and replicated when the objective is used again. This eliminates the need for manual re-adjustment of light intensity.

● **Nosepiece rotating buttons**

The nosepiece can be rotated allowing you to keep your eyes on the specimen. Your two favorite magnifications can be registered*, and one press of the button alternates between these two objective lenses. This is useful when frequent change of magnifications is necessary, for example between 10x and 40x objectives.

* Magnifications can be registered using the remote control pad's toggle mode.




● **Eco-illumination**

Provides streamlined observation with motorized operation

Motorized model with LED illumination

Equipped with motorized magnification switching and automatic intensity reproduction, it is ideally suited to applications and sample analysis that require frequent magnification switching.

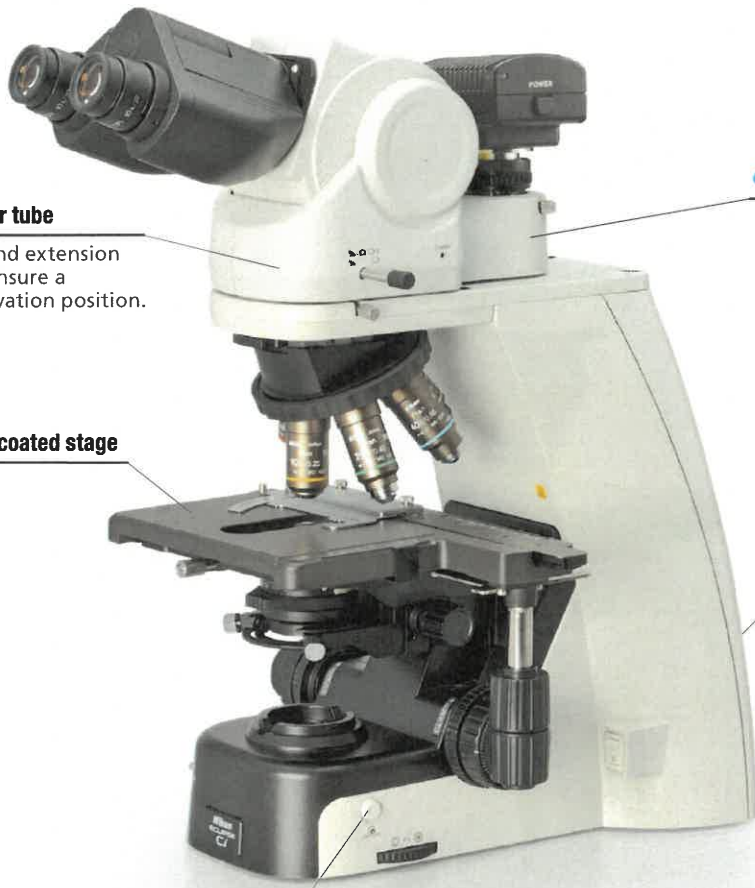

● **Ergonomic binocular tube**

Inclination angle and extension are adjustable to ensure a comfortable observation position.

● **DSC port**


A camera can be mounted to the ergonomic binocular tube via the optional DSC port.

● **Ceramic-coated stage**

● **Eco-illumination**

By combining a collimator lens, fly-eye optics and LED illumination, bright and uniform images up to the periphery can be obtained even in high magnification. The LED illuminator offers low-heat generation and provides the same color temperature in every magnification (patent pending).


● **Image capture button**

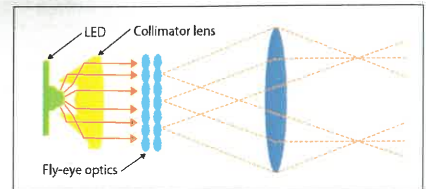

High-intensity and uniform Eco-Illumination

Manual model with LED illumination

Featuring Eco-illumination bright enough for phase contrast and simple polarizing microscopy while reducing lamp replacement with a long-life of 60,000 hours.

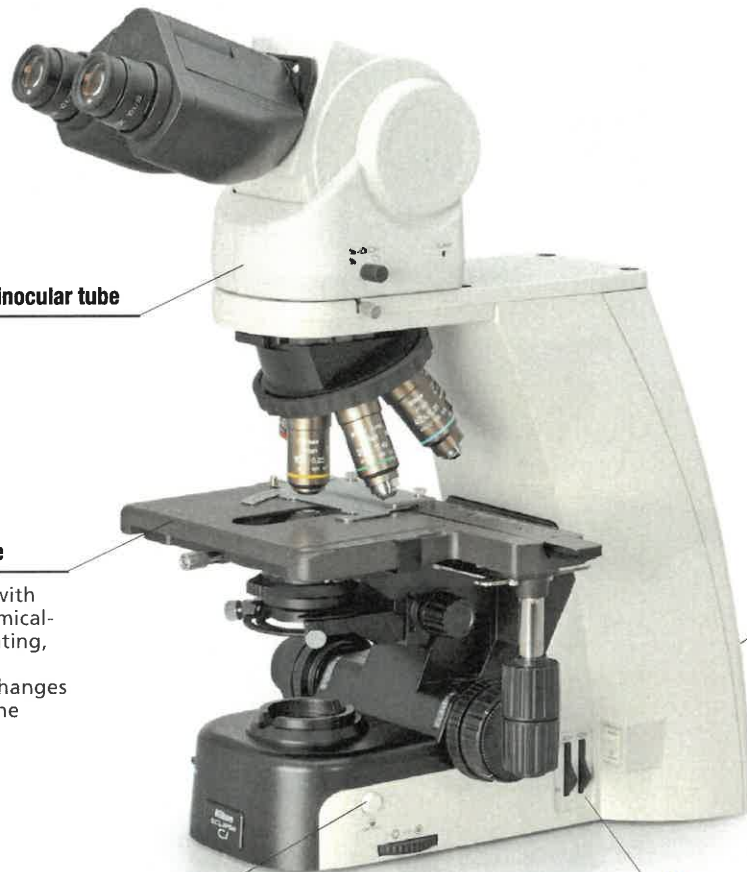

● **Ergonomic binocular tube**

● **Ceramic-coated stage**

The stage is coated with an abrasion and chemical-resistant ceramic coating, allowing long-term frequent specimen changes without damaging the stage surface.

● **Image capture button**

● **Space-saving compact design**

The compact body with an extremely small footprint gives the user more desk space than ever.

● **Halogen illumination**

● **ND4/ND8 filter, NCB11 filter**

Changing light intensity is possible by inserting and removing an ND (Neutral Density) filter. The NCB filter for color temperature compensation of the light source is built-in.


Enhanced basic performance for observation

Manual model with halogen illumination


With a small footprint and superior operability the ECLIPSE Ci series offers a comfortable, ergonomic viewing position.

Versatile observation techniques


Using accessories, the Ci-E, Ci-L and Ci-S enable various observation techniques to meet the demands of a wide range of uses, from clinical examination to research.

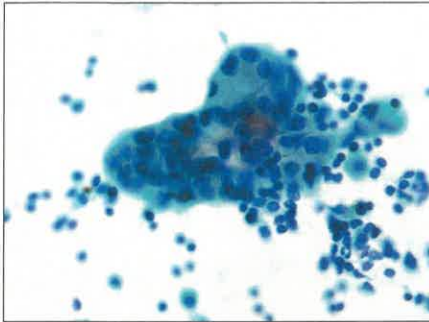

1 Breast Cancer, Pleural effusion, Papanicolaou stain, CFI Plan Apochromat Lambda 60XC

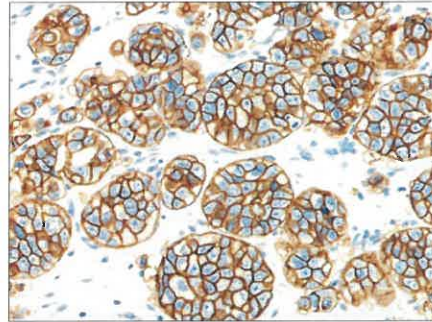


2 Breast Cancer, HER2/neu, Immunostaining, CFI Plan Apochromat Lambda 40X

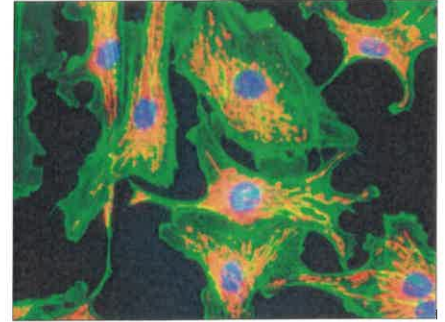


Epi-fluorescence


1 2 Photos courtesy of: Dr. Yoji Urata, Department of Diagnostic Pathology, Japanese Red Cross Kyoto Daiichi Hospital

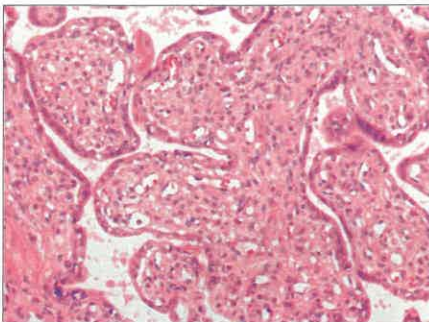

3 Human Placenta, HE stain, CFI Plan Apochromat Lambda 10X

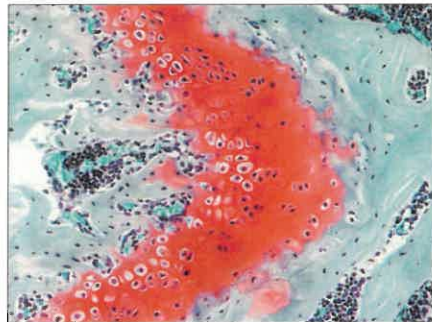


4 Cartilage of mouse femur, Safranin O fast green iron hematoxylin stain, CFI Plan Apochromat Lambda 10X

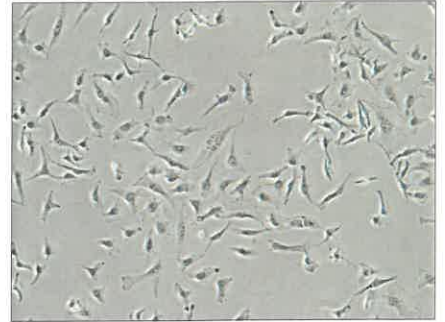


Phase contrast

3 4 Photos courtesy of: Dr. Atsushi Furuhashi and Noriyoshi Sueyoshi, Assistant General Manager, Laboratory of morphology and image analysis, Graduate School of Medicine, Juntendo University

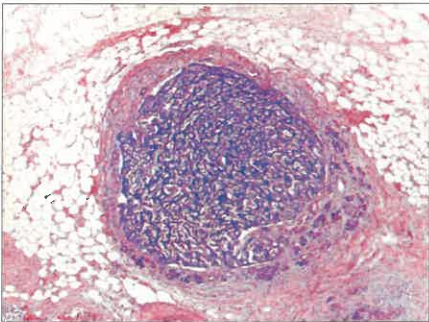

5 Pancreas Neuro-endocrine Tumor, HE stain, CFI Plan Apochromat Lambda 4X

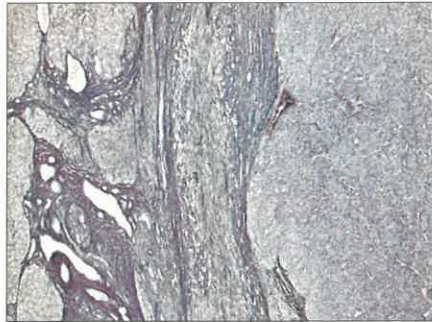


6 HCC, Silver stain, CFI Plan Apochromat Lambda 4X




Darkfield

5 6 Photos courtesy of: Kazuhiro Muraoka, Photography Division, Imaging Information Research Center, Tokyo Women's Medical University

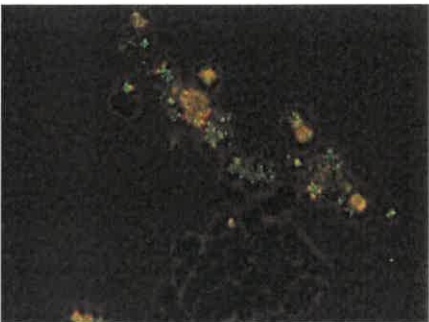

7 2,8-Dihydroxyadenine crystals, Simple polarizing, CFI Plan Fluor 40X

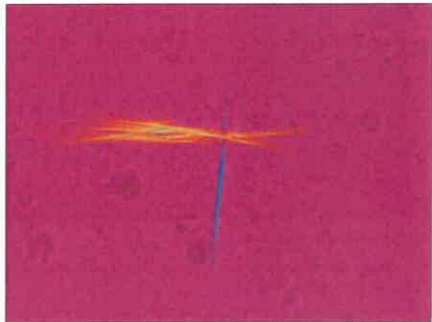

8 Sodium urate crystals, Sensitive color polarizing, CFI Plan Fluor 40X

7 8 Photos courtesy of: Department of Clinical laboratory, Nihon University Itabashi Hospital

Digital imaging evolved

In response to user demand for the easy capture of sample images, the ECLIPSE Ci series has a built-in dedicated capture button on the microscope base. An optional digital imaging system supports simple camera settings and operation including capturing, measuring and image sharing.


Image capture button

Image capturing with the digital camera Digital Sight series is possible with the one-touch button located on the microscope base, thereby improving workload efficiency.



DS-L4 Microscope Camera Control Unit

The DS-L4 tablet-style control unit eliminates the need and space requirements of a desktop PC to control DS-Ri2 and DS-Fi3 cameras. The touch panel allows the simple setting and operation of cameras by simply choosing the observation technique using scene mode icons. Simple measurement functions, such as distance measurement between two points, are available. Objective lens switching and a condenser setting of Ci-E are also possible.

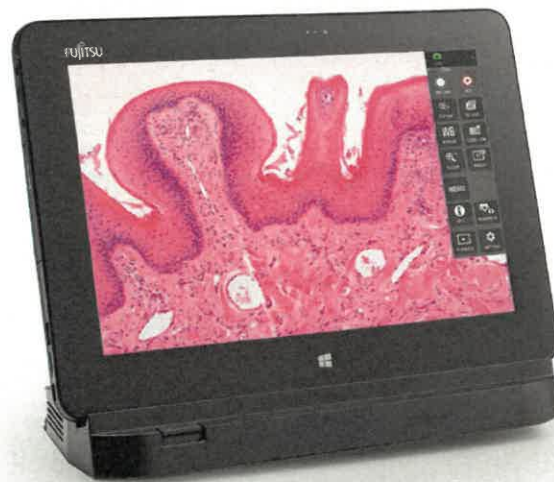

Scene mode icons

Optimal camera setting for each observation technique is possible by simply choosing an icon of the observation technique.



Camera setting

Simple camera setting is possible using icons. The numbers and layout of displayed icons can be customized.



Camera/microscope control

Objective lens switching and condenser setting of the Ci-E are possible.



Simple measurement

Simple measurement such as distance measurement between two points is possible.

Observation image sharing


During observation using the ECLIPSE Ci series microscope, live and captured images can be easily shared via the monitor of the DS-L4 microscope camera control unit, a projector, or a computer monitor*¹. In addition, connecting the ECLIPSE Ci series to a remote PC on the network easily enables remote viewing, online education, and distance collaboration.

*1 Requires a projector or PC monitor with FHD (1080p) or higher.

Digital pathology via a network

Connecting a Digital Sight series digital camera to the DS-L4 microscope camera control unit or a PC makes image sharing between multiple PCs on the network easy.

In essence, this unique network addressable system is the most powerful tool for consulting within or between hospitals as well as presentations and conferences during academic meetings, in-class lectures and distance education.

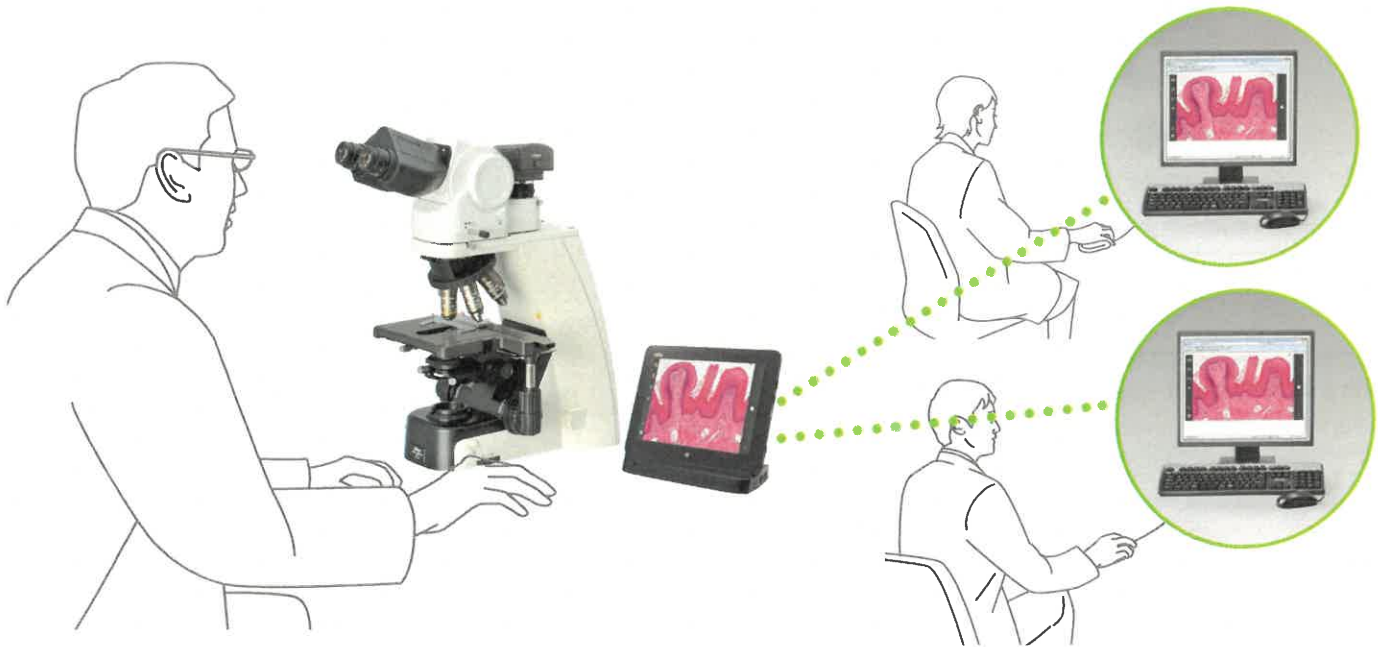

Digital Sight series microscope cameras

Nikon provides digital cameras that are optimized for microscopic imaging. Users can select the most suitable camera for their samples and observation techniques.

Microscope Camera DS-Fi3



5.9 megapixel

Color

High-definition

Equipped with a 5.9 megapixel CMOS image sensor. Enables fast and easy acquisition of images with superior color reproduction and high sensitivity during various observations, such as brightfield, DIC, phase contrast and epi-fluorescence.

Microscope Camera DS-Ri2



16.25 megapixel

Color


High-definition

Equipped with FX-format 16.25-megapixel CMOS sensors, the DS-Ri2 is perfect for capturing ultra-fine structures. It enables brightfield imaging with superior color reproduction and fast frame rates, as well as high sensitivity fluorescent imaging.

Ci accessories meet additional demands of

I want to observe using fluorescent microscopy.

The ECLIPSE Ci series has the option of two dedicated compact epi-fluorescence attachments, CI-FL Epi-fluorescence Attachment (4 filter cubes mountable) and D-FL Epi-fluorescence Attachment (6 filter cubes mountable).



I want to use phase contrast microscopy with LED illumination.

Eco-illumination has sufficient light intensity for phase contrast microscopy that is used in a wide range of applications including dermatological examinations.



Phase contrast accessories

I want to perform gout tests.


Eco-illumination is compatible with sensitive color polarizing microscopy, and gout tests can be conducted by observing uric acid crystals.



Sensitive color polarizing accessories

I want to observe specimens with a wider field of view.

Attaching the CFI UW 10X eyepiece lens with an F.N. of 25mm in combination with a trinocular tube T and trinocular tube F enables wide field microscopy.

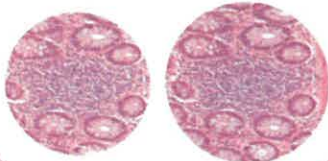

22mm

25mm

I want to reduce the number of times I switch the condenser.

An optional achromat swing-out condenser is compatible with a wide range of magnifications, between 1X to 100X.



I want to easily capture digital images of my specimens.

You can mount a camera on a trinocular tube T, trinocular tube F or an ergonomic binocular tube. Imaging in a comfortable position is possible with an ergonomic binocular tube by mounting the camera via the DSC port. Imaging is possible by simply pushing the image capture button.



Trinocular tube T

Trinocular tube F

Ergonomic binocular tube

I want to undertake long-term observation with minimal discomfort.

The ergonomic binocular tube can be inclined from 10° to 30° and extended up to 40mm.

The eyelevel riser lifts the tube in 25mm increments (up to 100mm*).

* Up to 50mm with ergonomic binocular tube.



Eyelevel riser

I want to observe the same view field simultaneously with another person


The teaching head enables multiple peoples to observe the same specimen simultaneously. A bright and long-life LED is employed in the pointer.

* 3-person type and 5-person type are also available.



Side-by-side type

Face-to-face type

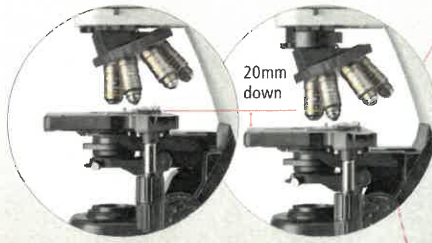

Without spacer

With spacer

I want more user-friendly stage operation.

The stage height can be lowered 20mm from the standard position by adding a nosepiece spacer, facilitating frequent specimen change.

The stage handle height can be changed to ensure a comfortable hand position.



I want to be able to quickly and safely change the specimen.

The stage height can be locked using the re-focusing knob, and this facilitates safe refocusing after changing the specimen.

I want to use various objective lenses.


Nikon provides a broad range of objective lenses, such as the CFI Plan Achromat series, which is affordably priced and has high image flatness, the CFI Plan Fluor series, which is suitable for fluorescence microscopy, and the CFI Plan Apochromt Lambda series, with its superior resolution, brightness and chromatic aberration correction.



Left: CFI Plan Achromat series; middle: CFI Plan Fluor series; right: CFI Plan Apochromt Lambda series



Ci System Diagram

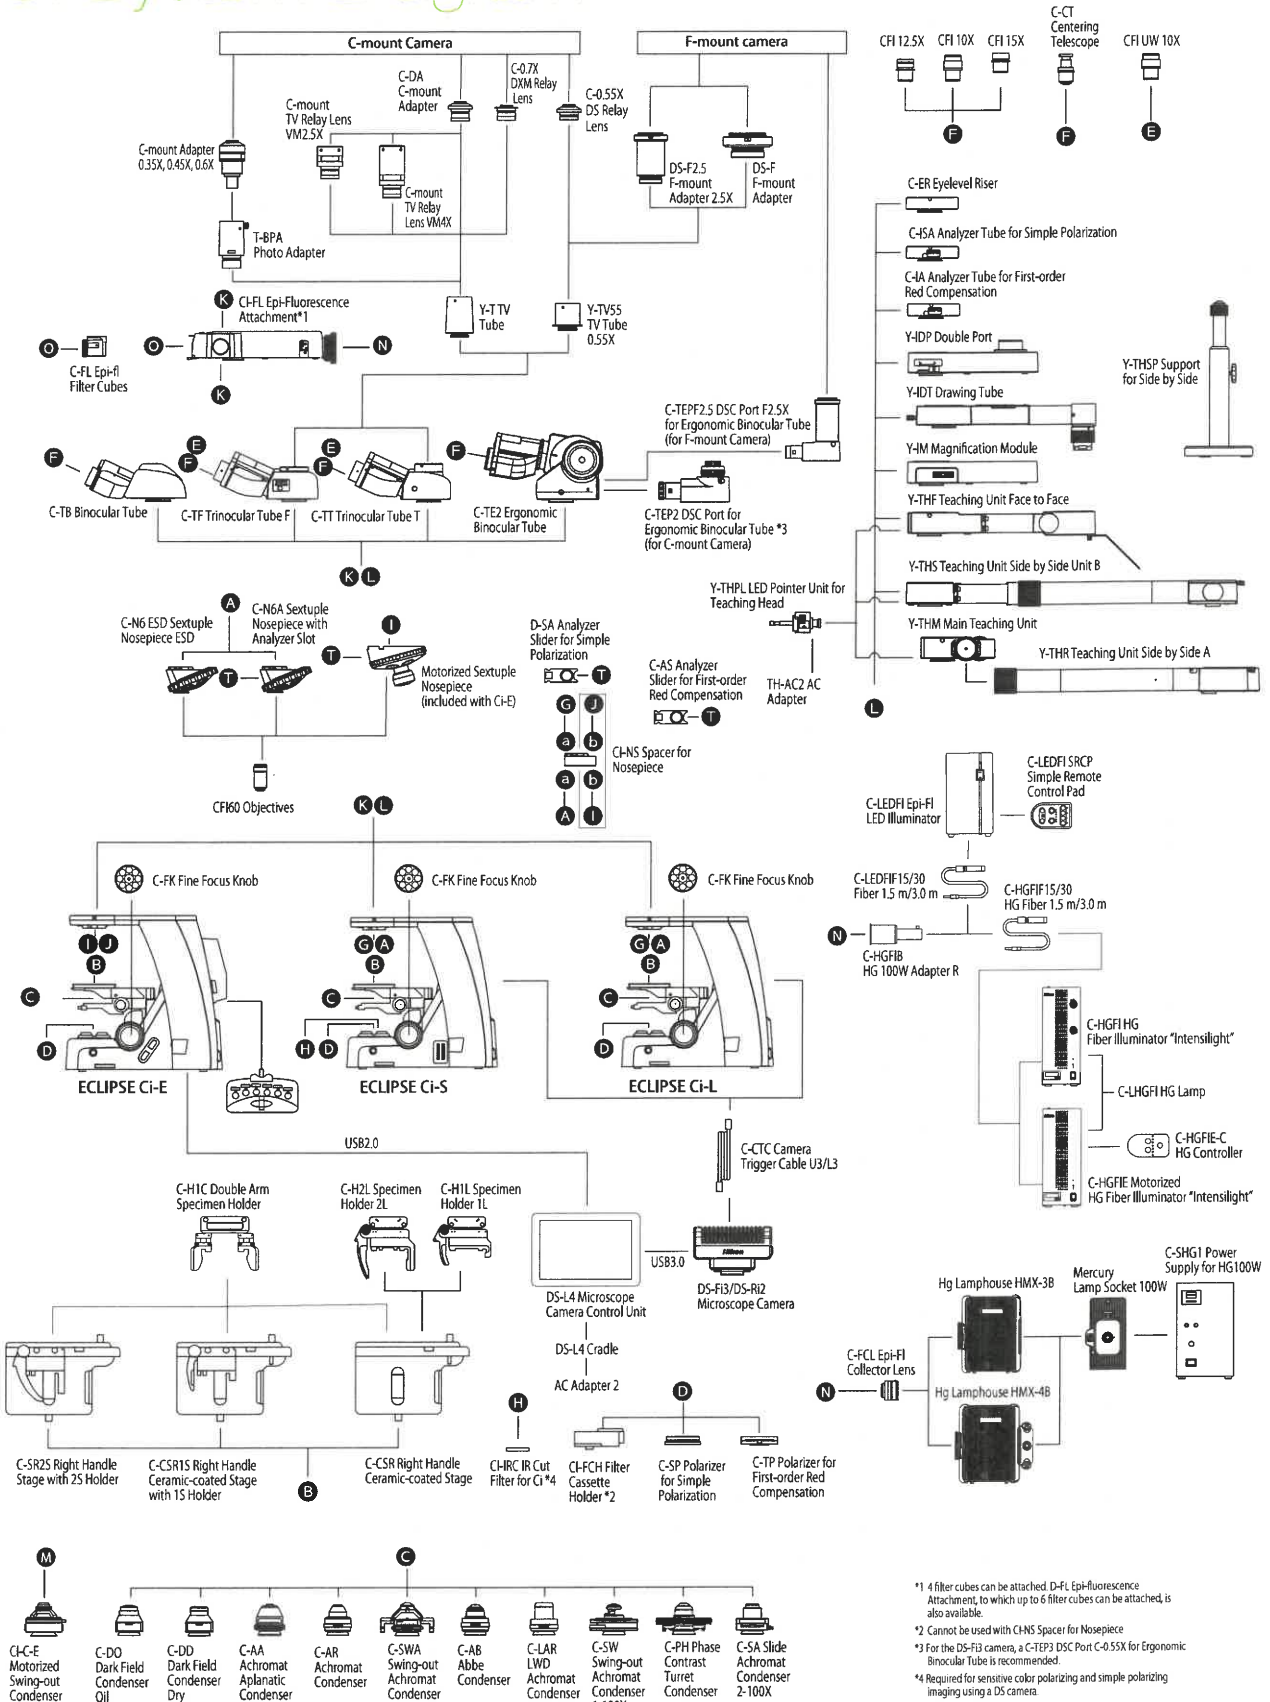

Specifications

		Ci-E	Ci-L	Ci-S
Main body	Optical system	CFI60 Infinity Optical System		
	Illumination	High luminescent White LED Illuminator (Eco-illumination)		6V30W Halogen Lamp Built-in ND4, ND8, NCB11 filters
		Automatic intensity reproduction function	—	
	Controls	Image capture button		
		Nosepiece rotating buttons Remote control pad	—	ND filter IN/OUT switches
Eyeieces (F.O.V. mm)	· CFI 10X (22) · CFI 12.5X (16) · CFI 15X (14.5) · CFI UW 10X (25)			
Focusing	Coaxial Coarse/Fine focusing, Focusing stroke: 30 mm, Coarse: 9.33 mm/rotation, Fine: 0.1 mm/rotation Coarse motion torque adjustable, Refocusing function			
Tubes	F.O.V. 22 mm (Eyepiece/Port)	· C-TB Binocular Tube · C-TE2 Ergonomic Binocular Tube (100/0, 50/50 via optional C-TEP2 DSC Port or C-TEPF2.5 DSC Port F2.5X) Inclination angle: 10-30 degree, Extension: up to 40 mm		
	F.O.V. 25 mm (Eyepiece/Port)	· C-TF Trinocular Tube F (100/0, 0/100) · C-TT Trinocular Tube T (100/0, 20/80, 0/100)		
Nosepieces	· Motorized Sextuple Nosepiece with Analyzer Slot (Within main body) Switching between two objectives function		· C-N6 ESD Sextuple Nosepiece ESD · C-N6A Sextuple Nosepiece with Analyzer Slot	
Stages	Cross travel 78 (X) × 54 (Y) mm, with vernier calibrations, stage handle height and torque adjustable for all stages C-H1C Double Arm Specimen Holder is available as an option for the below three stages. · C-SR2S Right Handle Stage with 2S Holder · C-CSR15 Right Handle Ceramic-coated Stage with 1S Holder · C-CSR Right Handle Ceramic-coated Stage (C-H2L Specimen Holder 2L and C-H1L Specimen Holder 1L can be attached)			
Condensers (NA)	Motorized	· CI-C-E Motorized Swing-out Condenser (0.90/0.22) Focusing stroke: 27 mm		
	Manual	Focusing stroke: 27 mm · C-AB Abbe Condenser (0.90) · C-AR Achromat Condenser (0.80) · C-DO Darkfield Condenser Oil (1.20-1.43) · C-DD Darkfield Condenser Dry (0.80-0.95) · C-PH Phase Contrast Turret Condenser (0.90) · C-AA Achromat/ Aplanat Condenser (1.40) · C-SA Slide Achromat Condenser 2-100X (0.90) · C-SW Swing-out Achromat Condenser 1-100X (0.90/0.11) · C-SWA Swing-out Achromat Condenser 2-100X (0.90/0.22) · C-LAR LWD Achromat Condenser (0.65)		
Observation methods*	Brightfield, Epi-fluorescence, Darkfield, Phase contrast, Simple polarizing, Sensitive color polarizing			
Epi-fluorescence attachment	· CI-FL Epi-fluorescence Attachment (4 filter cubes mountable) · D-FL Epi-fluorescence Attachment (6 filter cubes mountable) ND4/ND8/ND16 filters, Noise Terminator mechanism			
Epi-fluorescence light source	· C-LEDFl Epi-Fl LED Illuminator · C-HGFI/HGFIE HG Precentered Fiber Illuminator Intensilight (130W) · Hg Lamphouse and Power Supply (100W)			
Power consumption	13W (Brightfield configuration)		6W (Brightfield configuration)	38W (Brightfield configuration)
Weight (approx.)	15.4 kg (Binocular standard set)		13.4 kg (Binocular standard set)	13.4 kg (Binocular standard set)

*Observations except Brightfield require optional accessories.

Dimensional Diagram

Unit: mm

